


2.7 mm TPLO System


VAR-4027S

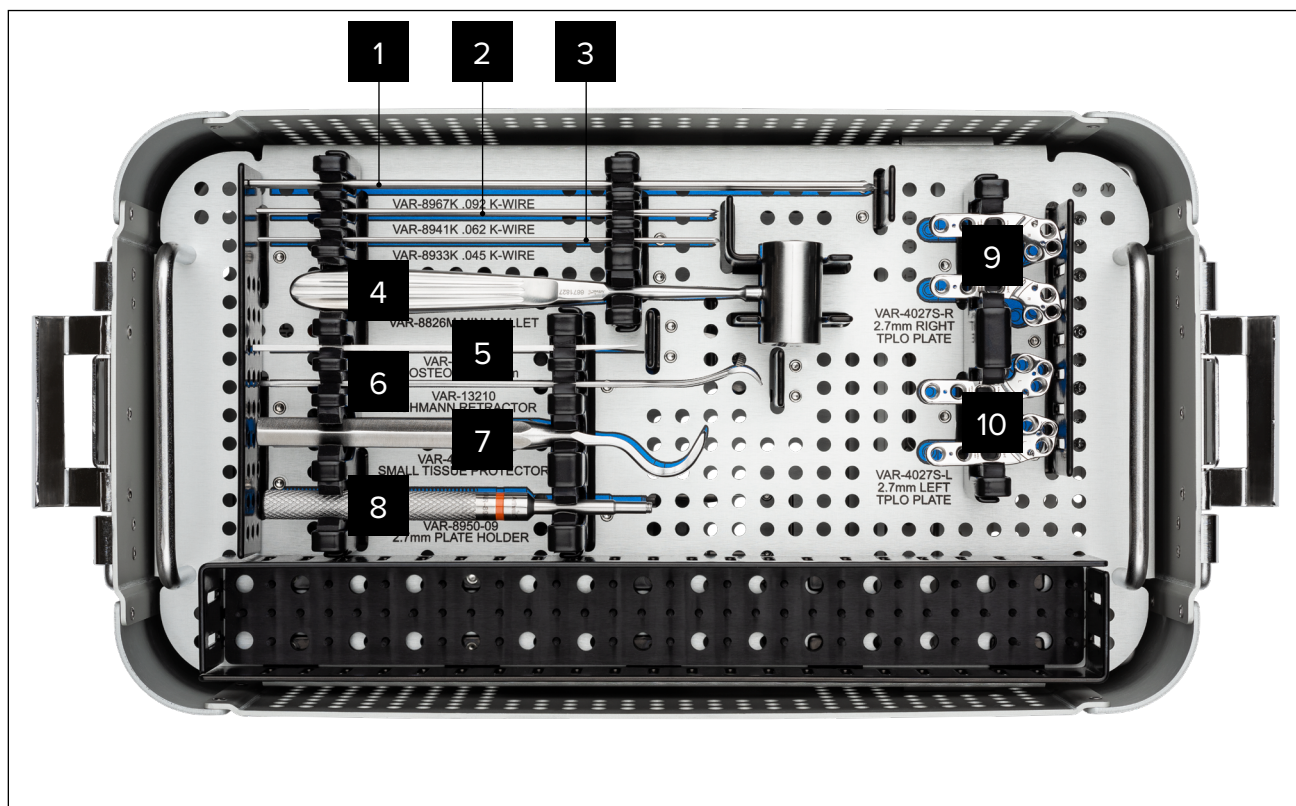

| Pic. | Item Number | Qty. | Description |
|------|--------------|------|---|
| 1 | VAR-8967K | | K-Wire, .092 in (2.3 mm) |
| 2 | VAR-8941K | | K-Wire, .062 in (1.57 mm) |
| 3 | VAR-8933K | | K-Wire, .045 in (1.14 mm) |
| 4 | VAR-8826M | | Mini Mallet, 7 in |
| 5 | VAR-13203-05 | | Small Osteotome, 5 mm |
| 6 | VAR-13210 | | Low Profile Hohmann Retractor |
| 7 | VAR-4000TPSM | | TPLO Tissue Protector, small |
| 8 | VAR-8950-09 | | Locking Plate Holder, 2.7 mm |
| 9 | VAR-4027S-R | | TPLO Locking Plate, 2.7 mm, standard, right |
| 10 | VAR-4027S-L | | TPLO Locking Plate, 2.7 mm, standard, left |

2.7 mm TPLO System

VAR-4027S

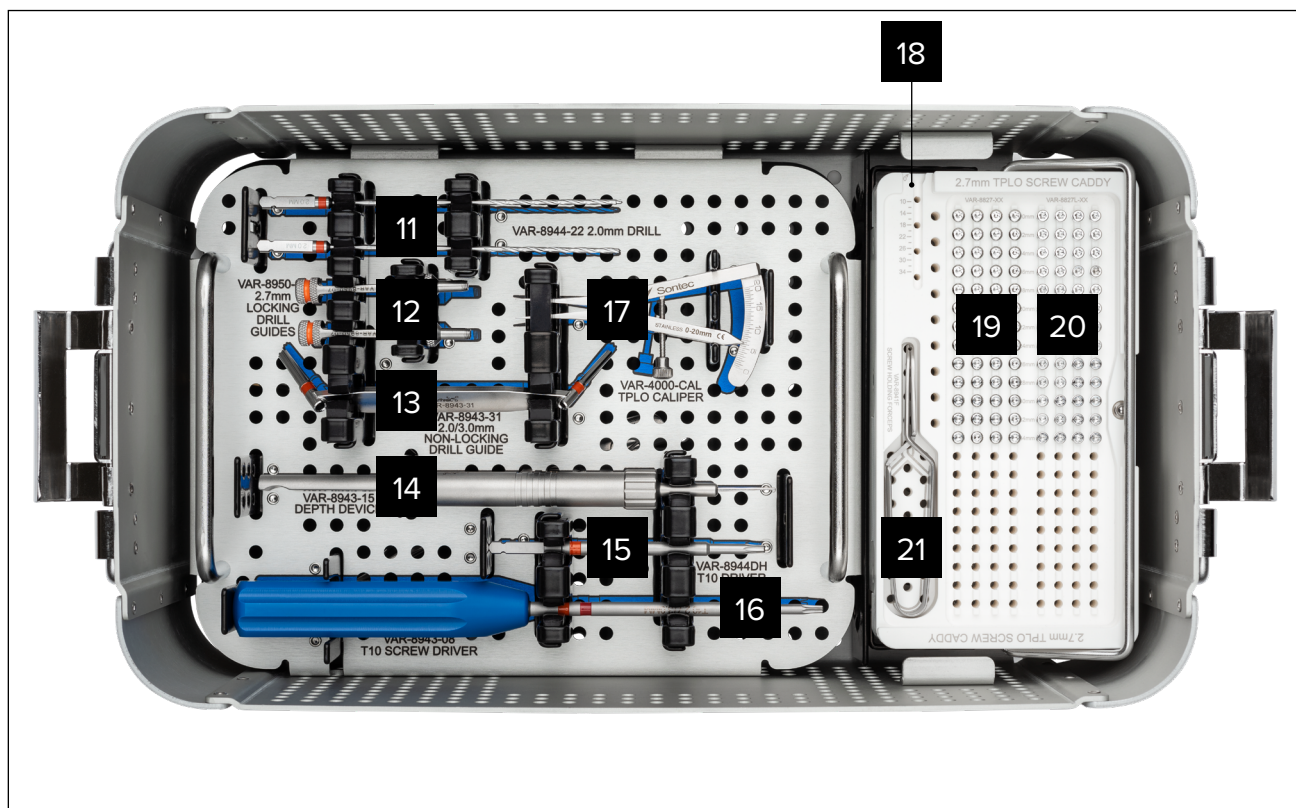

| Pic. | Item Number | Qty. | Description |
|------|---------------------|------|---|
| 11 | VAR-8944-22 | | Drill Bit, 2.0 mm |
| 12 | VAR-8950-07 | | Locking Drill Guide, 2.7 mm |
| 13 | VAR-8943-31 | | Nonlocking Drill Guide, 2.0 mm/3.0 mm |
| 14 | VAR-8943-15 | | Depth Device, low profile, 2.7 mm/3.5 mm |
| 15 | VAR-8944DH | | T10 Driver |
| 16 | VAR-8943-08 | | T10 Screwdriver |
| 17 | VAR-4000-CAL | | TPLO Caliper |
| 18 | VAR-4027SC-01 | | TPLO Screw Caddy, 2.7 mm |
| 19 | VAR-8827-10 to -34 | | Low-Profile Cortical Screw, 2.7 mm × 10 mm to 34 mm |
| 20 | VAR-8827L-10 to -34 | | Low-Profile Locking Screw, 2.7 mm × 10 mm to 34 mm |
| 21 | VAR-8941F | | Screw Holding Forceps |

2.7 mm TPL0 System

VAR-4027S

Date of Surgery:

Surgeon Name:

Account:

Representative Contact Information:

Set Total:

Miscellaneous Notes:

To obtain a copy of a product's directions for use (DFU), which includes sterilization instructions, please visit our website at www.arthrex.com/edfu or contact your local representative.

Page 3 of 3

www.arthrexvetsystems.com

© 2019 Arthrex, Inc. All rights reserved. vDOC1-000144-en-US_A

Arthrex[®]
CANINE
InternalBrace™ SYSTEM


Arthrex[®]
Vet Systems